

## Highly Selective and Sensitive Thiocyanate PVC Membrane Electrodes Based on Modified Zeolite ZSM-5

Atefeh Badri\*, and Pouya Pouladsaz

Department of Chemistry, Islamic Azad University, Shahreza Branch, P.O. Box 311-86145, Shahreza, Isfahan, Iran

\*E-mail: [atefebadri@gmail.com](mailto:atefebadri@gmail.com)

Received: 12 June 2011 / Accepted: 11 July 2011 / Published: 1 August 2011

---

A highly selective membrane electrode based on surfactant modified zeolite is presented. The proposed electrode shows very good selectivity for thiocyanate ions over a wide variety of common inorganic and organic anions. The sensor displays a near Nernstian slope of  $-58.9 \pm 0.9$  mV per decade. The working concentration range of the electrode is  $1.00 \times 10^{-6}$  -  $1.10 \times 10^{-1}$  M with a detection limit of  $8.33 \times 10^{-7}$  M. The response time of the sensor in whole concentration ranges is very short (<10 s). The response of the sensor is independent on the pH range of 2.0–10.1. The best performance was obtained with a membrane composition of 25.5% PVC, 64.5% dioctyl phthalate, 10% modified zeolite ZSM-5. It was successfully applied to direct determination of thiocyanate in water samples and as an indicator electrode for titration of thiocyanate ions with  $\text{AgNO}_3$  solution.

---

**Keywords:** Thiocyanate, Surfactant modified zeolite ZSM-5 (SMZ), potentiometry, Ion selective membrane electrode (ISE), Poly vinyl chloride (PVC)

### 1. INTRODUCTION

A very interesting development in the field of ion-selective electrodes (ISEs) is the construction of electrodes that can chemically recognize specific anions (chemo selectivity) and offer potentiometric responses that differ from the conventional anion-exchanger-based membranes. The quick determination of trace quantities of ionic species by simple methods is of special interest in analytical chemistry. Construction and application of ion-selective electrode as a potentiometric sensor offers interesting advantages such as simplicity, relatively fast response, low cost, wide linear dynamic range and ease of preparation and procedures. These characteristics have inevitably led to the preparation of numerous sensors for several ionic species, and the list of available electrodes has grown substantially over the past years [1].

Thiocyanate finds many industrial applications and though not as toxic as cyanide, it is harmful to aquatic life. Its determination at low levels in water and industrial effluents is therefore important. Thiocyanate sensors are potentially useful for detecting this compound in biological samples (e.g. urine and saliva), where elevated levels of thiocyanate correlate with excessive cigarette smoking. If the content of thiocyanate ion is a little higher in the body than normal, the protein dialysis will be affected and it may even result in coma. Due to the urgent need for selective potentiometric determination of trace amounts thiocyanate ion, especially in food, biological and water samples, many coordination compounds have been employed as an ionophore in the construction of ISEs thiocyanate ion [2–10].

Recent decade scientific researches introduced several PVC based sensors for different anions, such as  $\Gamma^-$  [11–13],  $\text{SCN}^-$  [3, 4, 9],  $\text{SO}_4^{2-}$  [14–19],  $\text{ClO}_4^-$  [20],  $\text{NO}_2^-$  [21, 22].

In this work, we report the use of a surfactant-modified zeolite ZSM-5 as an excellent ionophore for the preparation of a highly selective and sensitive polymeric membrane sensor for thiocyanate ion. The proposed sensor resulted in selectivity coefficients superior to those reported for other thiocyanate-selective electrodes.

## 2. EXPERIMENTAL

### 2.1. Reagents and chemicals

Sodium silicate used was the product of Merck and its composition is  $\text{SiO}_2$  (25.2–28.5%),  $\text{Na}_2\text{O}$  (7.5–8.5%),  $\text{H}_2\text{O}$  (63%). Chloridric acid (37%), sulfuric acid (98%), sodium hydroxide (98%), tetrapropylammonium bromide (TPABr 98%), Aluminum sulfate eighteen hydrate (>99.3%), sodium chloride (99.5%) were supplied from Merck.

The polymeric matrix was prepared from high relative molecular weight polyvinyl chloride (PVC). Reagent grade dioctylphthalate (DOP), tetrahydrofuran (THF) and hexadecyltrimethylammonium bromide (HDTMABr) were purchased from Aldrich or Fluka and used as received. Sodium and potassium salts of all anions were of the highest purity available (all from Merck) and used without any further purification. The pH of solutions was adjusted with sodium hydroxide or hydrochloric acid solution as appropriate. All other reagents used were of analytical reagent grade. De-ionized water was used throughout the experiments. A 0.1M stock solution of thiocyanate was prepared by dissolving an appropriate, accurate amount of KSCN. The standard  $1.0 \times 10^{-7}$ – $1.0 \times 10^{-1}$ M solutions of thiocyanate were prepared daily by sequential dilution of the appropriate stock solution with doubly distilled water.

### 2.2. Synthesis and modification of ZSM-5 zeolite

2.4984 g (0.0427 mol) of sodium chloride and 0.5931 g (0.00089 mol) of hydrated aluminum sulfate, were dissolved in 10.1200 g (0.5622 mol) of distilled water. 1.8945 g (0.00712 mol) tetrapropylammonium bromide, 7.1200 g (0.3955 mol) of distilled water and 1.0883 g (0.01088 mol)

sulfuric acid were added with vigorous stirring. 15.0000 g (0.07125 mol SiO<sub>2</sub>) of sodium silicate solution was subsequently added and the mixture was stirred for 60 min. The pH of the mixture was 9.38. The mixture was transferred into the autoclave. The autoclave was kept into an oven at 110 °C for about 2 h. Then, the temperature was increased to 230 °C and kept at that level for another 5 h. The solid phase obtained was filtered out, washed with water several times, dried at 110 °C for about 12-14 h and subsequently calcined at 540 °C for 3 h [23].

For preparation of surfactant modified zeolite (SMZ), the Na-ZSM-5 zeolite (2 g) was mixed with 100 mL of 50 mM HDTMA solutions, and stirred for 24 h on a magnetic stirrer. The mixture was then centrifuged at 5000 rpm for 20 min and the resulting SMZ was dried in air.

### 2.3. Characterization of the synthesized zeolite and the SMZ

The X-ray diffraction patterns of zeolite ZSM-5 was determined using a Bruker diffractometer, D8ADVANCE, X-ray tube anode: Cu, wavelength: 1.5406 Å (Cu K $\alpha$  radiation), filter: Ni. Fourier transformation infrared (FT-IR) spectra of samples, on KBr pellets, were recorded with a Nicolet single beam FT-IR (Impact 400D) spectrometer in the range of 400-4000 cm<sup>-1</sup>. All samples were stored in a desiccator until the FT-IR analysis and KBr of spectrometry grade was also heated at 25 °C to remove the adsorbed water before pressing. Then 1mg dry powdered sample was mixed with 100 mg KBr, followed by compressing the mixture to pellets with 12 mm diameter and investigating by the FT-IR spectrometer.

### 2.4. Electrode preparation

The procedure to prepare the best PVC membrane was to mix thoroughly 25.5 mg of powdered PVC, 10.0 mg of SMZ as ionophore and 64.5 mg of plasticizer DOP. Then the mixture was dissolved in 3 mL of dry THF. The resulting clear mixture was evaporated slowly until an oily concentrated mixture was obtained. A Pyrex tube (5 mm i.d.) was dipped into the mixture for about 10 s so that a nontransparent membrane of about 0.3 mm thickness is formed. The tube was then pulled out from the mixture and kept at room temperature for about 2 h. The tube was then filled with internal solution (1.0 $\times$ 10<sup>-2</sup> M KSCN). The electrode was finally conditioned for 16 h by soaking in a 1.0 $\times$ 10<sup>-2</sup> M KSCN solution. A silver/silver chloride electrode was used as an internal reference electrode. The electrode was instantly ready for use.

### 2.5. Potentiometric measurements

The potentiometric measurements were performed with a Metrohm pH meter 691 pH/ION Meter (Metrohm) at 25.0  $\pm$  1°C. A SMZ-membrane thiocyanate-selective PVC electrode and a standard Ag/AgCl electrode shielded by an intermediate salt-bridge compartment, containing the background electrolyte in order to prevent any transfer of potassium ions into the measuring solution, were used as an indicator electrode and an external reference electrode, respectively. All potentials

were reported versus this reference electrode. The cells for millivolt measurements were of the following type:

Ag/AgCl, KCl (3M) | internal solution KSCN ( $1.0 \times 10^{-2}$  M) | electrode membrane | test solution | Ag/AgCl, KCl (3M)

The potential reading of each solution was recorded when it became stable, and then plotted as a logarithmic function of  $\text{SCN}^-$  anion concentration. The activities of anions were based on the activity-coefficient data ( $\gamma$ ) calculated from the modified form of Debye-Huckel Equation [24], which is applicable to any ion and is as follows:

$$\log \gamma = -0.511Z^2 \left[ \frac{\mu^{1/2}}{(1+1.5\mu^{1/2})-0.2\mu} \right] \quad (1)$$


where  $\mu$  is the ionic strength and  $Z$  is the valency. All measurements were carried out at room temperature. The pH measurements were performed using a corning model 125 pH meter equipped with a combined electrode.

### 3. RESULTS AND DISCUSSION

#### 3.1. Synthesized zeolite and SMZ characterization

##### 3.1.1. X-ray diffraction studies

Synthesized ZSM-5 zeolite was characterized by X-ray diffraction.

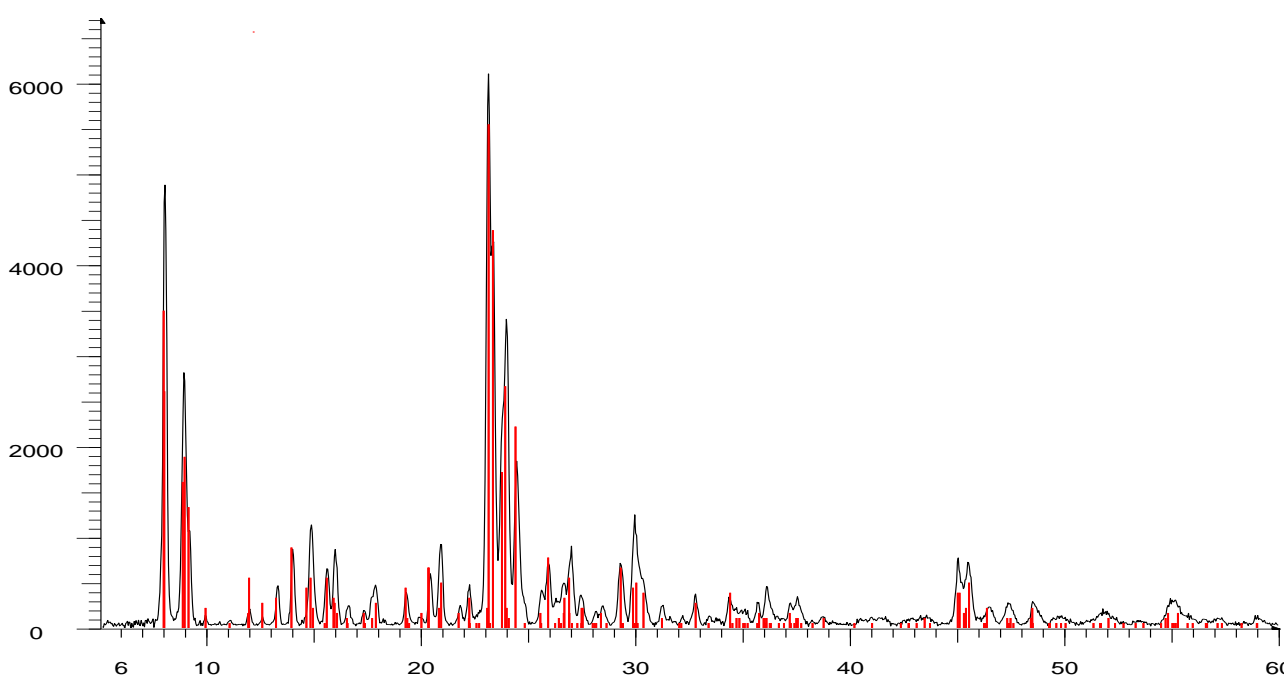

**Figure 1.** XRD patterns synthesized zeolite ZSM-5.

Figure 1 shows representative XRD patterns of sample synthesized. The measurements were conducted in continuous  $\theta/2\theta$  scan refraction mode. The anode was operated at 30 KV and 15 mA the  $2\theta$  angles were measured  $5^\circ-60^\circ$  at the rate of  $2^\circ.\text{min}^{-1}$ . The characteristic lines at  $2\theta$  of 7.9, 8.8, 23.1, 23.8 and 24.5 are observed from XRD pattern that show a good agreement with the data of Na- ZSM-5 zeolite [25]. The crystallinity of the prepared sample was calculated using the ratio of the sum of the areas of the most intense peaks for zeolite ZSM-5 sample (in above mentioned  $2\theta$  values) to the same peaks for the standard (zeolite ZSM-5) and multiplying by 100. This analysis shows that the product has a typical zeolite ZSM-5 structure with no amorphous material.

3.1.2. FT-IR studies

FT-IR lattice vibration spectra were used to investigate the influence of surfactant on the zeolite framework.

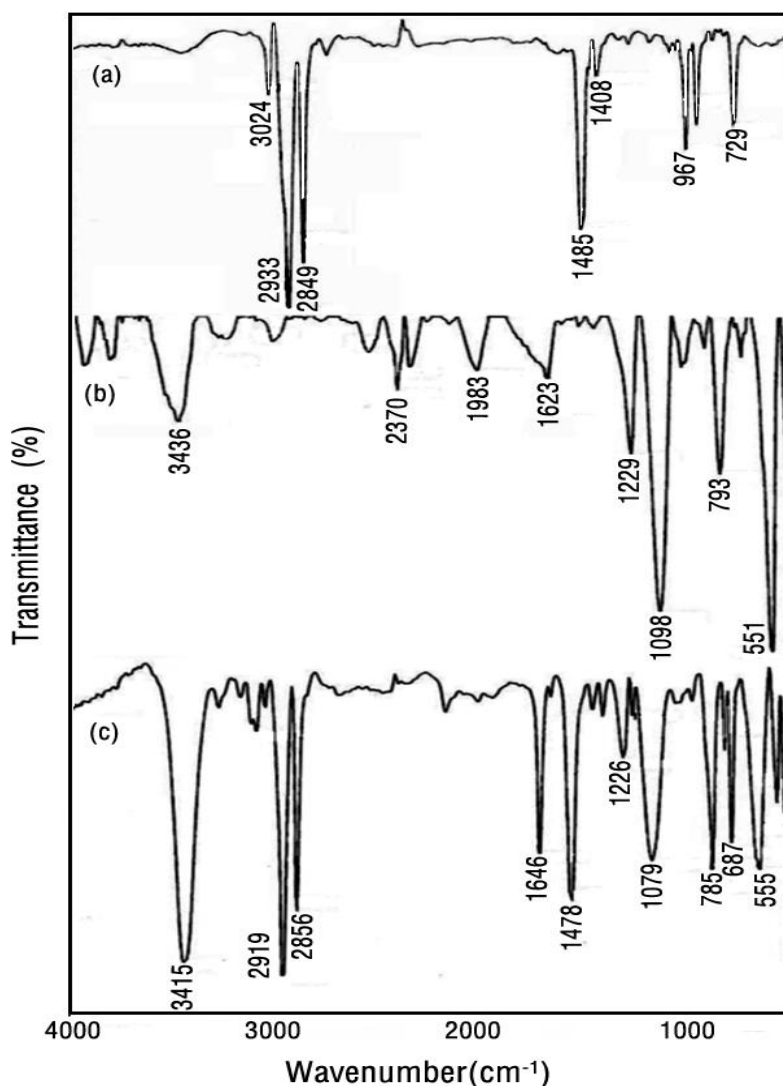


Figure 2. FT-IR patterns for (a) HDTMA (b) synthesized ZSM-5 and (c) SMZ.

Representative spectra of zeolite HDTMA, ZSM-5 and SMZ in the range of 400–4000 $\text{cm}^{-1}$  are shown in Fig. 2. According to Fig. 2b, the observed frequencies at 3436, 1623, 1098 and 551 $\text{cm}^{-1}$  agrees with the infrared spectral data, which has been obtained for zeolite ZSM-5 by Flanigen *et al.* [26]. The IR pattern of SMZ-ZSM-5 shows characteristic peaks at 2919, 2856, 1478 and 687  $\text{cm}^{-1}$  in fig. 3c, which indicate the incorporation of HDTMA into the zeolite structure. There is a slight shift in peaks at each wavenumber, however, both of the patterns are nearly the same. Specially, the presence of peaks at 2919, 2856 and 1478  $\text{cm}^{-1}$  in SMZ spectrum (related to C-H, C-C and N-C vibrations in the surfactants, respectively), that are absent in the Na- ZSM-5 spectrum, confirm loading of HDTMA on zeolite surface.

### 3.2. Theoretical considerations of SMZ and electrode behavior

As previously mentioned, the SMZ can be used for sorption of anionic species. This is based on the conceptual model which was illustrated graphically in the previous work [27]. At low concentrations, HDTMA forms a monolayer on the zeolite surface with the hydrophobic ends of the molecules turned toward the solution. With increasing coverage, a second HDTMA layer is also formed. This bilayer structure causes arrangement of positively charged functional groups toward the solution, which can serve as sorption sites for anions [28]. Complete formation of the second layer, means that sorbed HDTMA concentration is twice of the external cation exchange capacity (ECEC).

Preliminary experiments showed that when SMZ is mixed with a solution containing thiocyanate anion, the concentration of thiocyanate in the remaining solution is decreased. Therefore, we were prompted to use the SMZ as an active ingredient for construction of a potentiometric sensor for this anion. The sorption mechanism can be shown by the following reaction:



where  $\text{R}_4\text{N}^+$  represents the anion-exchange sites of HDTMA surfactant on SMZ. According to the above discussions, when proposed electrode is immersed in thiocyanate solutions, anion exchange reaction takes place between anions on the electrode surface ( $\text{Br}^-$ ) and  $\text{ClO}_4^-$  in solution.

### 3.3. Optimization of the membrane composition

In preliminary studies, some experiments regarding the response towards mono and divalent anions were carried out. Except with  $\text{SCN}^-$  ion, the E versus pM plots is nonlinear within the concentration range of  $1.0 \times 10^{-1}$  to  $1.0 \times 10^{-7}$  M, and exhibit hypo-Nernstian slopes (table 1). Our preliminary experiments showed that the membrane prepared by using the zeolite ZSM-5 as ion sensing proved to be suitable one, and all of optimizations were done on SMZ-PVC electrode. First, the amount of SMZ modifier was optimized. The responses of the electrodes to several SMZ compositions are presented in Table 2. As can be seen, only the electrode containing 10% SMZ which was prepared from Na-ZSM-5 at 50 mM HDTMA, as described in section 2.2, showed Nernstian

behavior. Electrodes which were prepared at 100 and 200 mM HDTMA solution do not show a Nernstian behavior.

**Table 1.** Potentiometric response of the electrode toward different anions (n=4).

Anion	Slope(mV.decade <sup>-1</sup> )	r <sup>2</sup>	Linear range (-log C)
ClO <sub>4</sub> <sup>-</sup>	46.7 ± 0.8	0.9809 ± 0.08	5.2-1.1
ClO <sub>3</sub> <sup>-</sup>	36.1 ± 0.9	0.9903 ± 0.08	5.0-3.1
SO <sub>4</sub> <sup>2-</sup>	19.2 ± 1.1	0.9393 ± 0.04	4.8-2.1
SO <sub>3</sub> <sup>2-</sup>	20.2 ± 0.9	0.9807 ± 0.07	5.1-1.9
C <sub>2</sub> O <sub>4</sub> <sup>2-</sup>	17.1 ± 0.9	0.9866 ± 0.04	4.8-1.9
I <sup>-</sup>	41.2 ± 0.8	0.9791 ± 0.08	5.1-2.6
NO <sub>3</sub> <sup>-</sup>	18.1 ± 0.8	0.9870 ± 0.008	4.1-2.1
HPO <sub>4</sub> <sup>2-</sup>	30.4±1.4	0.9678 ± 0.009	5.1-2.0
SCN <sup>-</sup>	60.7 ± 1.6	0.9933 ± 0.005	6.6-1.2
Br <sup>-</sup>	34.3 ± 0.9	0.9661±0.004	4.8-2.0

**Table 2.** Optimization the modifier amount.

Electrode	Modifier percentage	Slope (mV. decade <sup>-1</sup> ) (n=5)
A	4%(NaZSM-5+100 mM HDTMA)	<b>-42.0 ± 1.1</b>
B	10%( NaZSM-5+100 mM HDTMA)	<b>-53.1 ± 0.5</b>
C	15%( NaZSM-5+100 mM HDTMA)	<b>-45.1 ± 0.7</b>
D	4%( NaZSM-5+200 mM HDTMA)	<b>-42.5 ± 0.8</b>
E	10%( NaZSM-5+200 mM HDTMA)	<b>-53.1 ± 0.5</b>
F	15%( NaZSM-5+200 mM HDTMA)	<b>-56.1 ± 0.8</b>
G	4%( NaZSM-5+50 mM HDTMA)	<b>-40.1 ± 1.1</b>
*H	10%( NaZSM-5+50 mM HDTMA)	<b>-58.7 ± 0.3</b>
I	<b>15%( NaZSM-5+50 mM HDTMA)</b>	<b>-41.1 ± 0.8</b>

**Table 3.** Composition and potentiometric characterization of thiocyanate selective electrode based on SMZ-PVC membrane (n=4).

No	PVC%	SMZ%	DOP%	Average Slope (mV.decad <sup>-1</sup> )	r <sup>2</sup>	Linear range(-log C)	RSD
1	29	4.0	67	53.4±1.2	0.9910 ± 0.0030	5.5-1.0	3.2
*2	25.5	10.0	64.5	58.6±0.9	0.9960 ± 0.0190	6.0-1.1	1.7
3	23.5	15.0	61.5	44.3±1.3	0.9711 ± 0.0200	4.4-1.1	4.3
4	21	20.0	59	39.2±0.8	0.9701 ± 0.0141	3.9-1.2	2.9


In this case, a partially formed bilayer may be loaded on the zeolite surface. Consequently, the obtained SMZ does not respond appropriately to SCN<sup>-</sup>. This completely agrees with the results which

were obtained by Wingenfelder et al. [29] for antimonate sorption studies. They found that, in the treatments about two times of the ECEC, the zeolite took up over 98% of the initial HDTMA in solution. When the applied HDTMA concentrations were over two times as high as the ECEC, the zeolite took up 84% of the initial HDTMA concentration.

The potential response of a sensor is greatly related to the membrane ingredients [30-34]. The ratio of membrane ingredients were optimized so that the membranes develop reproducible, noiseless and stable potentials. Composition of the membranes, which resulted in the best performance, is shown in Table 3 along with their potentiometric characteristics. As it can be seen, electrodes made from membranes containing 10% (w/w) zeolite in the presence of 25.5% polymer, 64.5% dioctylphthalate were found to be the optimum one in the development of this sensor (membrane no. 2, Table 3). Thus, this membrane composition was used for subsequent works.

### 3.4. Effect of internal reference solution

The concentration of the internal solution (KSCN) in the electrode was changed from  $1.0 \times 10^{-2}$  to  $1.0 \times 10^{-4}$  M and the emf-pSCN<sup>-</sup> plots were obtained and the results are shown in Fig. 3.

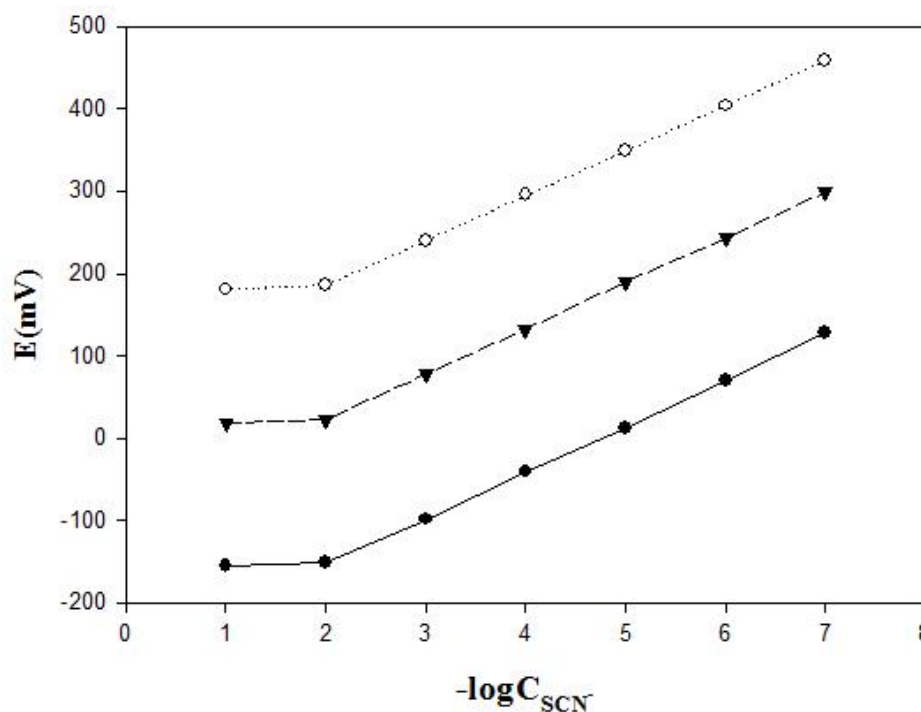

**Figure 3.** Effect of concentration of internal reference solution on the electrode response at various thiocyanate concentrations in the range of  $1.0 \times 10^{-1}$  M- $1.0 \times 10^{-3}$  M.

It was found that the variation of the concentration of the internal KSCN solution did not cause any significant difference in potential response except for an expected change in the intercept of the resulting plots. A  $1.0 \times 10^{-2}$  M concentration of internal reference solution is quite appropriate for




smooth functioning of the electrode system. Then conditioning time was studied by changing the time of being electrode in conditioning situation (Table 4). The obtained results showed the best Nernstian behavior was for 16 h.

**Table 4.** Conditioning time results for SMZ-PVC membrane electrode (10% modifier;  $-\log C = 6 - 2$ ; ( $n=5$ )).

t (h)	Slope (mV.decade <sup>-1</sup> )	r <sup>2</sup>
4	38.0 ± 0.9	0.9893 ± 0.0377
6	39.9 ± 1.6	0.9877 ± 0.0438
8	40.9 ± 0.9	0.9699 ± 0.0069
10	46.7 ± 0.4	0.9899 ± 0.0066
12	49.9 ± 0.9	0.9901 ± 0.0038
*16	59.3 ± 0.9	0.9870 ± 0.0080
18	52.4 ± 0.9	0.9982 ± 0.0723
24	53.8 ± 1.2	0.9191 ± 0.0132
48	55.5 ± 0.9	0.9694 ± 0.0066

### 3.5. Effect of pH

The influence of pH of the test solution ( $1.0 \times 10^{-3}$  M thiocyanate) on the potential response of the SMZ-membrane sensor was tested in the pH range 1.1–13.1 (adjusted with either HCl or NaOH) and the results are shown in Fig. 4.

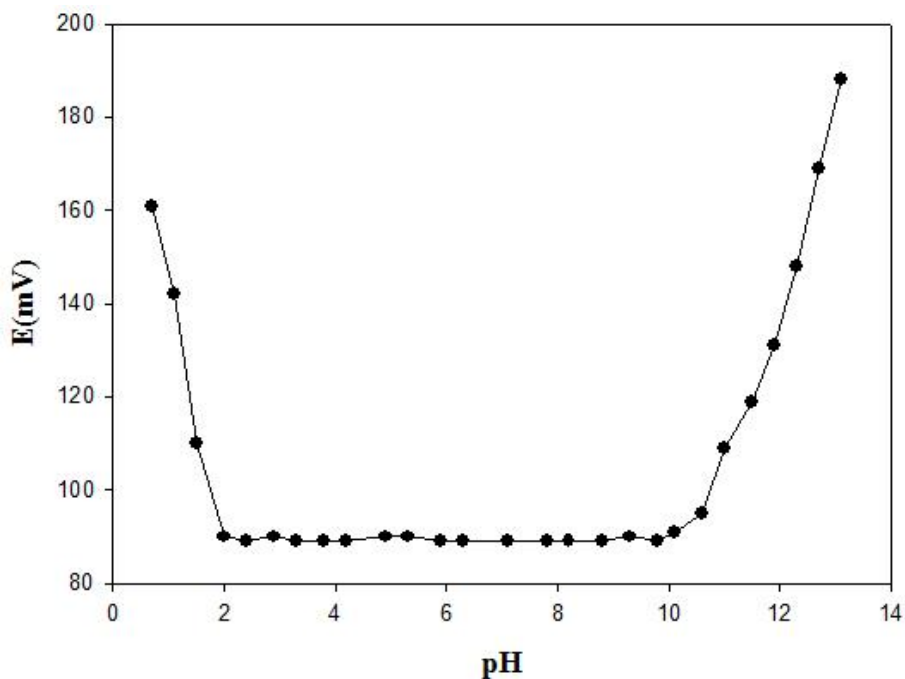

**Figure 4.** Influence of pH on the potential response of the thiocyanate-selective electrode to  $1.0 \times 10^{-2}$  M SCN<sup>-</sup>.

As seen, the membrane electrode can be suitably used in the pH range 2.0–10.1. A pH of 6.0 was adjusted with 0.1 mol L<sup>-1</sup> acetic acid-acetate buffer was used for further studies. However, drastic potential changes are observed at higher and lower pH values. This is most probably due to the simultaneous response of the electrode to SCN<sup>-</sup> and OH<sup>-</sup>, at pH > 10.1, and some ionophore protonation and consequent diminished responsivity to SCN<sup>-</sup> and/or simultaneous response to thiocyanate and chloride ions, at pH < 2.0.

### 3.6. Effect of ionic strength on the response of the electrode

The effect of ionic strength (1.0×10<sup>-4</sup> to 3.4×10<sup>-3</sup> M NaNO<sub>3</sub>) on the calibration curve of the SMZ-PVC electrodes was investigated and the obtained results are listed in Table 5.

**Table 5.** Effect of ionic strength on optimized SMZ-PVC membrane electrode response.

Concentration of NaNO <sub>3</sub> (M)	Slope= $\bar{x}$ (n=6) (mV.decade <sup>-1</sup> )	t <sub>exp</sub>	Linear range of thiocyanate (M)	Intercept (mV)
1.0×10 <sup>-4</sup>	-59.1±0.56	0.040	1.00×10 <sup>-6</sup> -1.10×10 <sup>-1</sup>	236
3.0×10 <sup>-4</sup>	-59.5±0.76	1.18	1.00×10 <sup>-6</sup> -1.10×10 <sup>-1</sup>	235
4.9×10 <sup>-4</sup>	-59.3±0.61	0.73	1.00×10 <sup>-6</sup> -1.10×10 <sup>-1</sup>	233
1.0×10 <sup>-3</sup>	-59.5±0.66	0.95	1.00×10 <sup>-6</sup> -1.10×10 <sup>-1</sup>	232
2.0×10 <sup>-3</sup>	-59.7±0.78	1.43	1.00×10 <sup>-6</sup> -8.97×10 <sup>-2</sup>	197
3.4×10 <sup>-3</sup>	<b>-59.3±0.67</b>	<b>0.33</b>	<b>1.00×10<sup>-6</sup>-8.94×10<sup>-2</sup></b>	<b>190</b>

Note: t<sub>0.05,5</sub>=2.57 (Ref. 35)

The electrode response has a Nernstian slope with linear range of 1.00×10<sup>-6</sup>-1.10×10<sup>-1</sup> of thiocyanate anion within the 1.0×10<sup>-4</sup> to 1.0×10<sup>-3</sup> M of NaNO<sub>3</sub>. This was indicated by the constant Nernstian behavior and the same linearity range obtained at different ionic strength values. Nevertheless, within the 2.0×10<sup>-3</sup> to 3.4×10<sup>-3</sup> M NaNO<sub>3</sub>, the Nernstian slopes were obtained but the linear range decreased to 1.00×10<sup>-6</sup>-8.97×10<sup>-2</sup>M of thiocyanate anion. In higher concentrations (>1×10<sup>-3</sup> M NaNO<sub>3</sub>, results not showed) it is possible that some of the ion exchange sites in SMZ are occupied by NO<sub>3</sub><sup>-</sup> ions. As the result it causes a decrease in electrode response compare to the higher concentrations of the thiocyanate anions. The difference in the intercept values at nitrate concentrations lower than 1 mM is not significant. The small differences indicate that the sensor is free from nitrate interference at concentrations of nitrate lower than 1 mM. But, the intercept values at nitrate concentrations higher than 1 mM are more different and nitrate has much more interference. The validity of obtained results was performed by statistical methods. By comparing of t<sub>exp</sub> and t<sub>0.05,5</sub>=2.57 at 95% confidence interval it is concluded that there is a random error in experiments [35].

### 3.7. Effect of temperature

To investigate the thermal stability of the electrode, calibration curves ( $E_{\text{cell}}$  versus  $\log a_{\text{SCN}^-}$ ) were constructed at different temperatures covering the range 25–60 °C. The electrode exhibited good Nernstian behavior in the range of 25–45 °C. The results are shown in Table 6.

**Table 6.** Effect of temperature on optimized SMZ-PVC electrode behavior.

Temperature (°C)	Nernstian slope (mV.decade <sup>-1</sup> )	Mean of exp. slope (n=10), mV.decade <sup>-1</sup>	$t_{\text{exp}}$
25	-59.2	-59.6 ± 0.7	<b>1.81</b>
30	-60.2	-60.0 ± 0.8	<b>0.79</b>
35	-61.2	-61.5 ± 0.5	<b>1.90</b>
40	-62.2	-62.6 ± 0.6	<b>2.10</b>
45	-63.2	-63.6 ± 0.7	<b>1.81</b>
50	-64.2	-65.1 ± 0.6	<b>4.74</b>
55	-65.0	-67.2 ± 1.3	<b>5.35</b>
60	<b>-66.0</b>	<b>-67.9 ± 0.9</b>	<b>6.67</b>

Note:  $t_{0.05, 9} = 2.26$  (Ref. 35)

Experimental slope calculated from Eq. (3) which is applicable to any temperature:

$$\text{Nernstian slope} = 2.303 \times \frac{RT}{nF} \quad (3)$$


where  $n$  is the valancy,  $R$ ,  $T$  and  $F$  are the universal gas constant, the absolute temperature and the Faraday constant.

The Nernstian and experimental slope values at each temperature were compared statistically, showing conformity of the slopes for 10 replicates. The results prove the validation of the obtained results with the expected values in the temperature range of 25–45 °C. However, at temperatures higher than 45 °C the slopes show a significant deviation from the theoretical values. This deviation may be related to desorption of the surfactant from SMZ and destruction of the electrode surface.

### 3.8. Response time

The response time of the sensor was defined as  $t_{95}$  for the slope of the calibration curve of thiocyanate solution when the thiocyanate concentration was increased from  $1.0 \times 10^{-7}$  to  $1.0 \times 10^{-1}$  mol L<sup>-1</sup> (Fig. 5), where  $t_{95}$  is the time required for the sensor to reach 95% of the steady state (final signal that does not change during 60 s) potentiometric value. From the results, the best response time of 5 s was recorded for membrane having the optimized conditions. After new solutions were exposed to the electrode the response changed rapidly and remained at a constant value before 5 s of the exposure.

The potential generated by the membrane (when it's remained constant in one solution of thiocyanate) remained constant for 5 min, after which it started slow deviating ( $-0.5\%$  per min).

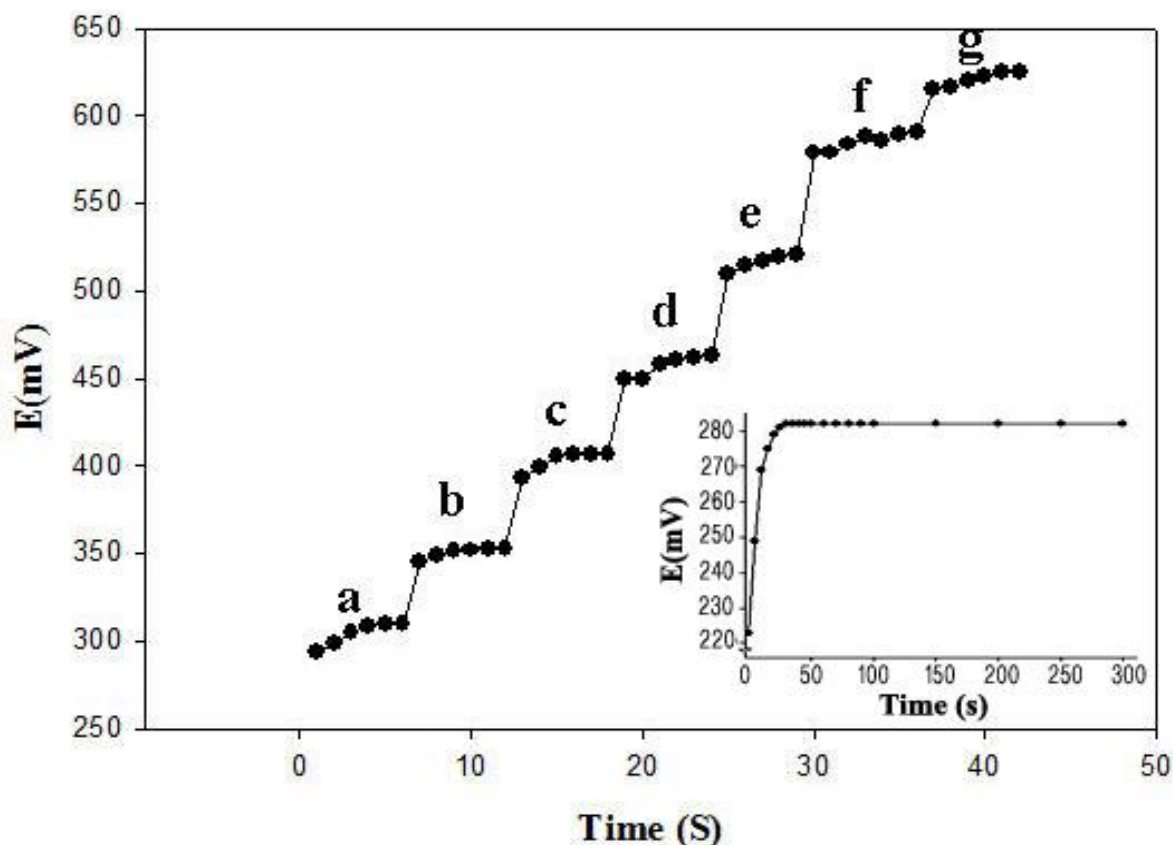

**Figure 5.** Response time of the SMZ-PVC to different concentration of thiocyanate (pH=5.5) in the range of  $1 \times 10^{-7}$  to  $6 \times 10^{-1}$  M (in sequence of “g” to “a” in figure), (Inset: Static response time of the proposed membrane electrode towards  $\text{SCN}^-$  ions)

The static response time of the membrane electrode thus obtained was  $<10$  s. The potential reading stays constant, to within  $\pm 1$  mV, for at least 5 min (the inset of Fig. 5).

### 3.9. Definition of interference (Selectivity coefficients)

Interference occurs when a substance or process leads to a false result in a measurement technique [36]. The influence of interfering ions on the response behavior of ion-selective membrane electrodes is usually described in terms of selectivity coefficients. Potentiometric selectivity coefficients ( $K_{\text{SCN}^-; \text{A}^-}^{\text{Pot}}$ ) describing the preference of the membrane for an interfering ion  $\text{A}^-$  relative to  $\text{SCN}^-$ . The experimental selectivity coefficients depend on the activity and the method of their determination. Different methods of selectivity determination have been found in the literatures. Potentiometric selectivity coefficient values for the present sensors were determined by the separate solutions method (SSM), according to IUPAC recommendations, using  $1.0 \times 10^{-3}$  M solutions of  $\text{SCN}^-$


and interfering ions. The potentiometric selectivity coefficients of the proposed electrode, in the optimized analytical procedure, are calculated using the following equation [37] and summarized in Table 7:

$$\log K_{\text{SCN}^-, j}^{\text{Pot}} = \frac{nF(E_j - E_i)}{2.303RT} + \log \left( \frac{a_i}{a_j^{n/m}} \right) \quad (4)$$

Where  $K_{\text{SCN}^-, A}^{\text{Pot}}$  is the potentiometric selectivity coefficient,  $E_i$  the measured cell potential at primary ion activity  $a_i$  ( $\text{SCN}^-$ ),  $E_j$  the measured cell potential at interference ion activity  $a_j$ ,  $n$  and  $m$  are the charges of the primary and interference ion, respectively.  $R$ ,  $T$  and  $F$  have their common meaning.

**Table 7.** Potentiometric selectivity coefficients of various interfering anions ( $n=4$ ).

Interfering anion	$\log K_{\text{ClO}_4}^{\text{Pot}} \pm \text{SD}$	Interfering anion	$\log K_{\text{ClO}_4}^{\text{Pot}} \pm \text{SD}$
$\text{ClO}_4^-$	$-0.9 \pm 0.08$	$\text{CN}^-$	$-3.1 \pm 0.09$
$\text{I}^-$	$-1.2 \pm 0.05$	$\text{CO}_3^{2-}$	$-2.6 \pm 0.06$
$\text{IO}_4^-$	$-2.1 \pm 0.07$	$\text{BrO}_3^-$	$-3.0 \pm 0.11$
$\text{ClO}_3^-$	$-2.8 \pm 0.07$	$\text{IO}_3^-$	$-3.1 \pm 0.21$
$\text{C}_2\text{O}_4^{2-}$	$-2.9 \pm 0.09$	$\text{Cl}^-$	$-3.3 \pm 0.11$
$\text{NO}_3^-$	$-1.9 \pm 0.10$	$\text{Br}^-$	$-2.5 \pm 0.10$
$\text{CH}_3\text{COO}^-$	$-3.4 \pm 0.07$	Salicylate	$-2.4 \pm 0.08$




As can be seen, of the different anions tested, the largest sensitivity was obtained for thiocyanate, perchlorate, iodide, nitrate and periodate. a poorer response was observed with salicylate and the responses to other anions were practically negligible.

The selectivity sequence follows the Hofmeister Series (the selectivity based solely on lipophilicity of anions) [38], ( $\text{ClO}_4^- > \text{SCN}^- > \text{I}^- > \text{NO}_3^- > \text{Br}^- > \text{Cl}^- > \text{HCO}_3^- > \text{CH}_3\text{COO}^- > \text{SO}_4^{2-} > \text{HPO}_4^{2-}$ ) although some slight deviations might be interpreted because of some preferential coordination of this ionophore with certain anions.

### 3.10. Response characteristics of the electrode

Using the optimized composition and conditions described above, the critical response characteristics of the electrode were assessed according to IUPAC recommendations [39]. The emf response of the electrode to varying concentrations of thiocyanate species indicates a linear range from  $1.00 \times 10^{-6}$  to  $1.10 \times 10^{-1}$  M ( $r = 0.9966$ ) (Fig. 6). The average slope of calibration curves based on 14 replicate measurements was  $-58.9 \pm 0.9$  mV per decade of  $\text{SCN}^-$  concentration. Comparison of this calculated value with theoretical Nernstian value (59.2 mV per decade of  $\text{SCN}^-$  concentration) by statistical ( $t$ ) parameter ( $t_{\text{calc}} = 1.87$  and  $t_{0.05,13} = 2.16$ ) shows that the difference between them is due to

random errors. On the other hand, the proposed SMZ membrane electrode is applicable to measure  $\text{SCN}^-$  anion in aqueous solutions. The lower and upper detection limits were  $8.33 \times 10^{-7}$  and 0.13 M, respectively.

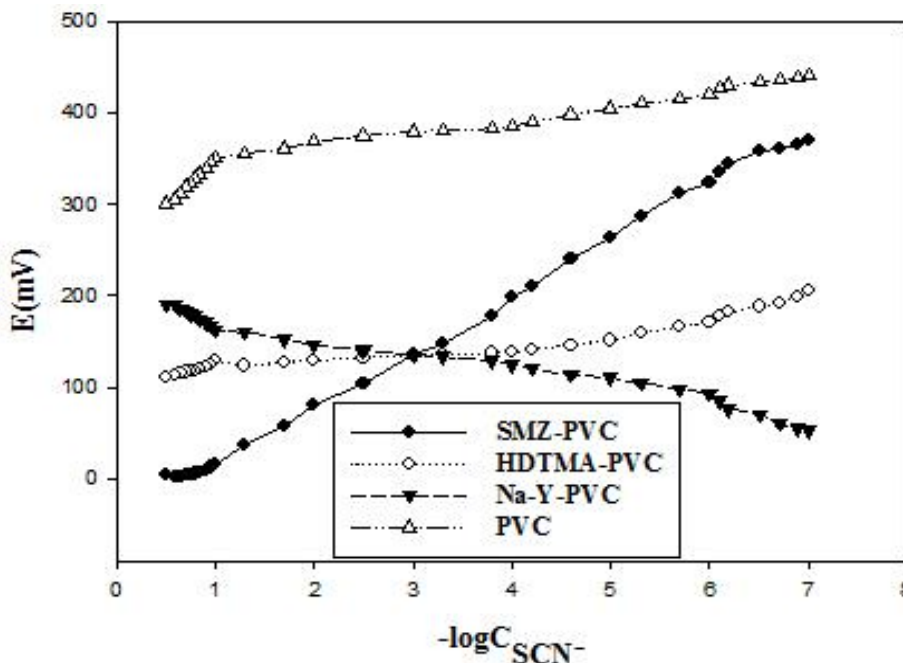

**Figure 6.** Potentiometric response of the proposed electrodes toward thiocyanate.

Long term stability of the electrode was investigated by taking the response of the optimized electrode in a period of 30 days. Potentiometric measurements were performed every day during the first week and then every three days for the rest of the period. The electrode retained its full activity during this period. The relative standard deviations (RSD) of a single electrode (within electrode variation) were determined every 30 s during a period of 0-120s, (n=5). This process was repeated 10 times. The RSD values were between 0.5 and 1.4%. The small relative standard deviations (0.2–1.0%) and hence good repeatability of the electrodes indicates that the PVC membrane is homogeneous.

The reproducibility of the potentiometric response of the optimized electrode was also investigated by carrying the measurements on four independent electrodes with the same composition. These measurements were also performed in 10 replicates. The obtained relative standard deviation (between electrode variations) was less than 1.5%. The validity of results was investigated by “g” value statistical test, g-test [35], as:

$$g = \frac{\text{highest } s^2}{s_1^2 + s_2^2 + \dots s_k^2} \tag{5}$$

Where  $s_i^2$  is the variance of each class of determinations. The calculated “g” values for each case was 0.4793 which are smaller than the critical g value at 95% confidence interval,  $g_{0.05,10,4} =$

0.5017 (4 class, 10 replicate in each class) [35] indicating that there is no significant difference between the behavior of the four independent electrodes and those compositions are homogeneous.

**Table 8.** Comparison of some characteristics of the proposed electrode with previous  $\text{SCN}^-$  ISEs.


Ref.	Slope ( $\text{mVdecade}^{-1}$ )	Working pH range	Linear range (M)	DL (M)	Ionophore
<b>Proposed electrode</b>	$-58.9 \pm 0.9$	2.0–10.1	$1.00 \times 10^{-6}$ – $1.01 \times 10^{-1}$	$8.33 \times 10^{-7}$	SMZ
[40]	-56.3	2.0–8.0	$6.0 \times 10^{-6}$ – $1.0 \times 10^{-2}$	$5.0 \times 10^{-6}$	Tetra-midopyridine
[40]	-58.3	2.0–8.0	$1.0 \times 10^{-5}$ – $1.0 \times 10^{-2}$	$5.0 \times 10^{-6}$	Hexa-imidopyridine
[41]	-57.0	5.0	$9.0 \times 10^{-7}$ – $1.0 \times 10^{-1}$	$7.0 \times 10^{-7}$	[Cu(II) <sub>2</sub> -BBSTA]
[42]	-56.5	3.5–8.5	$1.0 \times 10^{-6}$ – $1.0 \times 10^{-1}$	$7.0 \times 10^{-7}$	[Zn(BDSH)]
[43]	-58.7	3.0–8.0	$1.0 \times 10^{-5}$ – $1.0 \times 10^{-1}$	$4.0 \times 10^{-6}$	Rh[(trpy)(bpy)Cl](PF <sub>6</sub> ) <sub>2</sub>
[44]	-57.6	3.9–9.2	$1.0 \times 10^{-6}$ – $1.0 \times 10^{-1}$	$5.0 \times 10^{-7}$	CCT
[44]	-58.7	4.3–9.8	$1.0 \times 10^{-6}$ – $1.0 \times 10^{-1}$	$5.7 \times 10^{-7}$	NOBP
[45]	-52.0	2.0–3.0	$3.0 \times 10^{-5}$ – $1.0 \times 10^{-1}$	$2.5 \times 10^{-5}$	Calix[4]arene

Some response characteristics of the proposed electrode compared with other thiocyanate selective electrodes and the obtained results are summarized in Table 8. As can be seen from Table 8, in some cases, selectivity coefficient and dynamic linear range that were obtained for the proposed electrode are superior and comparable to those reported previously for other thiocyanate-selective membrane electrodes based on variety of different ionophores. It is important to note that in all cases in Table 8, response time, stability and electrode response independent pH range for the proposed SMZ-PVC are much better than those reported for other compared electrodes. The SMZ-PVC has applicability in a wide pH range (2.0–10.1), for acidic to basic solutions. High stability of the electrode is another advantage of proposed electrode that it in turn causes an increasing of precision. In investigation of reproducibility and repeatability, the RSD values for our SMZ-PVC (1.3–2.4%) are smaller than others (2–5%). This shows the SMZ-PVC has a better precision.

### 3.11. Practical application

The optimized membrane thiocyanate electrode was successfully used for potentiometric determination of  $\text{SCN}^-$  via  $\text{Ag}^+$  titrations. Fig. 7 shows the titration curve of 10mL of a  $1.0 \times 10^{-2}$  M thiocyanate solution titrated with  $1 \times 10^{-2}$  M of  $\text{AgNO}_3$ . The titration volume was measured at the inflection point of the titration curve and a concentration of thiocyanate of  $9.7 \times 10^{-3}$  M was determined.

The new thiocyanate -selective electrode was applied for the determination of thiocyanate in river and tap water samples with satisfactory results. The analysis was performed by using the standard addition technique. The results are summarized in Table 9. Good recoveries were obtained in all samples.

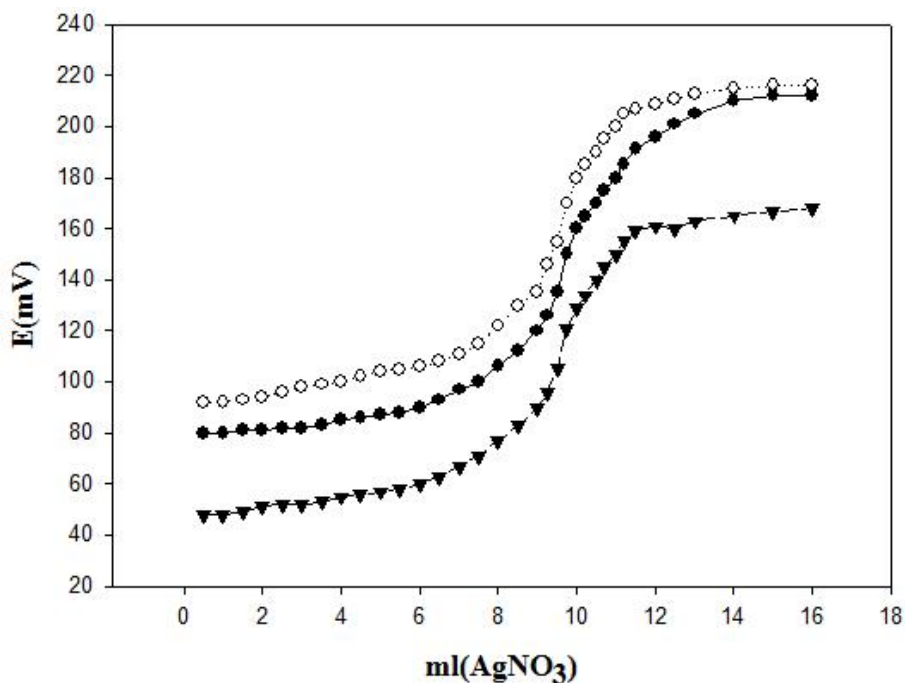

**Figure 7.** Potentiometric titration curve for 10 ml of  $1.0 \times 10^{-2}$  M  $\text{SCN}^-$  solution with  $1.0 \times 10^{-2}$  M  $\text{AgNO}_3$  using the proposed sensor as an indicator electrode ( $n=5$ ).

**Table 9.** Determination of thiocyanate in drinking and river water.

Recovery(%)	Foundet thiocyanate ( $\mu\text{g/ml}$ )	Added thiocyanate ( $\mu\text{g/ml}$ )	Samples
-	0	-	Tap Water of Isfahan
95.0	$1.33 \pm 0.21$	1.4	
93.5	$2.15 \pm 0.44$	2.3	
97.3	$2.92 \pm 0.32$	3.0	
98.1	$5.23 \pm 0.45$	5.3	
-	0	-	The River Water of Zayandeh Rood in Isfahan
100.6	$10.16 \pm 0.23$	10.1	
99.3	$15.14 \pm 0.55$	15.3	
99.1	$20.01 \pm 0.35$	20.2	
98.9	$25.12 \pm 0.88$	25.4	

#### 4. CONCLUSIONS

To sum up, we have shown that the use of the modified zeolite by cationic surfactant can be used as suitable ionophores in the development of new thiocyanate-selective PVC membrane electrodes. These electrodes show a Nernstian response, detection limits of near  $8.33 \times 10^{-7}$  M and a low response time of a few seconds in the presence of thiocyanate. The optimized membrane electrode was used as indicator electrode in potentiometric titrations of thiocyanate with silver.



## ACKNOWLEDGMENT

We wish to acknowledge the financial support from the Research Council of Islamic Azad University, Shahreza Branch.

## References

1. V. K. Gupta, R. N. Goyal, and R. A. Sharma, *Int. J. Electrochem. Sci.*, 4 (2009) 156
2. S. S. Hassan, M. H. Abou Ghalia, A. G. E. Amr, and A. H. K. Mohamed, *Anal. Chim. Acta*, 482 (2003) 9
3. T. Poursaberi, M. Salavati-Niasari, S. Khodabakhsh, L. Haji-gha Babaei, M. Yousefi, S. Rouhani, and M. R. Ganjali, *Anal. Lett.*, 34 (2001) 2621
4. M. R. Ganjali, T. Poursaberi, F. Basiripour, M. Salavati-Niasari, M. Yousefi, and M. Shamsipur, *J. Anal. Chem.*, 370 (2001) 1091
5. M. K. Amini, A. Rafi, M. Ghaedi, M. H. Habibi, and M. M. Zohory, *Microchem. J.*, 75 (2003) 143
6. A. Abbaspour, M. A. Kamyabi, A. R. Esmaeilbeig, and R. Kia, *Talanta*, 57 (2002) 859
7. M. M. Ardakani, A. A. Ensafi, M. Salavati-Niasari, and S. Mihoseini Chahooki, *Anal. Chim. Acta*, 462 (2002) 25
8. X. Huang, Y. Chai, R. Yuan, X. Wang, and Q. Li, *Anal. Sci.*, 20 (2004) 1185
9. M. R. Ganjali, M. Yousefi, M. Javanbakht, T. Poursaberi, M. Salavati-Niasari, L. Haji-gha Babaei, E. Latifi, and M. Shamsipur, *Anal. Sci.*, 18 (2002) 887
10. J. Y. Dai, Y. Q. Chai, R. Yuan, Y. S. Zhang, Y. Liu, X. Zhong, and D. P. Tang, *Chem. Lett.*, 34 (2005) 62
11. T. Poursaberi, M. Hosseini, M. Taghizadeh, H. Pirelahi, M. Shamsipur, and M. R. Ganjali, *Microchem. J.*, 72 (2002) 77
12. M. R. Ganjali, T. Poursaberi, M. Hosseini, M. Salavati-Niasari, M. Yousefi, and M. Shamsipur, *Anal. Sci.*, 18 (2002) 289
13. M. R. Ganjali, A. Daftari, F. Mizani, and M. Salavati-Niasari, *Bull. Korean Chem. Soc.*, 24 (2003)
14. M. Shamsipur, M. Yousefi, M. Hosseini, M. R. Ganjali, H. Sharghi, and H. Naemi, *Anal. Chem.*, 73 (2001) 2869
15. M. Shamsipur, M. Yousefi, M. R. Ganjali, T. Poursaberi, and M. Faal-Rastgar, *Sensor Actuator B*, 82 (2002) 105
16. M. R. Ganjali, V. Akbar, A. Daftari, P. Norouzi, H. Pirelahi, and A. Mouradzadegan, *J. Chin. Chem. Soc.*, 51 (2004) 309
17. M. R. Ganjali, M. Ghorbani, A. Daftari, P. Norouzi, H. Pirelahi, and H. D. Dargahani, *Bull. Korean Chem. Soc.*, 25 (2004) 172
18. M. R. Ganjali, F. Mizani, H. Pirelahi, M. Taghizadeh, and J. Amani, *Can. J. Anal. Sci. Spect.*, 47 (2002) 157
19. M. R. Ganjali, M. R. Pourjavid, M. Shamsipur, T. Poursaberi, M. Rezapour, M. Javanbakht, and H. Sharghi, *Anal. Sci.*, 19 (2003) 995
20. M. R. Ganjali, M. Yousefi, T. Poursaberi, L. Naji, M. Salavati-Niasari, and M. Shamsipur, *Electroanalysis*, 18 (2003) 1476
21. M. Shamsipur, M. Javanbakht, A. R. Hassaninejad, H. Sharghi, M. R. Ganjali, M. F. Mousavi, *Electroanalysis*, 15 (2003) 1251
22. M. R. Ganjali, M. Rezapour, M. R. Pourjavid, and M. Salavati-Niasari, *Anal. Sci.*, 19 (2003) 1127
23. M. Ghiaci, F. Seyedeyn-Azad, and R. Kia, *Mater. Res. Bull.*, 39 (2004) 1257
24. R. Buck, and V. Cosofret, *Pure Appl. Chem.*, 65 (1993) 1849
25. H. Robson, *Verified Syntheses of Zeolitic Materials*, Elsevier, Amsterdam, (2001)
26. E. M. Flanigen, H. Khatami, and H. A. Szymanski, *Molecular Sieve Zeolites Advances in Chemistry Series*, vol. 101, American Chemical Society, Washington, D. C., (1971)

27. A. Nezamzadeh-Ejhi, and N. Masoudipour, *Anal. Chim. Acta*, 658 (2010) 68
28. Z. Li, and R. S. Bowman, *Environ. Sci. Technol.*, 31 (1997) 2407
29. U. Wingenfelder, G. Furrer, and R. Schulin, *Micropor. Mesopor. Mat.*, 95 (2006) 265
30. M. R. Ganjali, P. Norouzi, A. Atrian, F. Faridbod, S. Meghdadi, and M. Giasi, *Mater. Sci. Eng. C*, 29 (2009) 205
31. V. K. Gupta, A. K. Jain and G. Maheshwari, *Int. J. Electrochem. Sci.*, 2 (2007) 102
32. M. R. Ganjali, R. Nemati, F. Faridbod, P. Norouzi, and F. Darviche, *Int. J. Electrochem. Sci.*, 3 (2008) 1288
33. V. K. Gupta, R. N. Goyal and R. A. Sharma, *Int. J. Electrochem. Sci.*, 4 (2009) 156
34. V. K. Gupta, M. Al Hayat, A. K. Singh and M. K. Pal, *Anal. Chim. Acta*, 634 (2009) 36
35. R. L. Anderson, *Practical Statistics for Analytical Chemists*, Van Nostrand Reinhold, New York, (1987)
36. G. Dimeski, *Clin. Biochem. Rev. Suppl (i)*, 29 (2008) 43
37. Y. Umezawa, P. Buhlmann, K. Umezawa, K. Tohda, and S. Amemiya, *Pure Appl. Chem.*, 72 (2000) 1851
38. F. Hofmeister, *Arch. Exp. Patol. Pharmacol.*, 24 (1988) 247
39. G. G. Guibault, R. A. Durst, M. S. Frant, H. Freiser, E. H. Hansen, T.S. Light, E. Pungor, G. Rechnitz, N. M. Rice, W. Simon, and J. D. R. Thomas, *Pure Appl. Chem.*, 48 (1976) 127
40. S. S. M. Hassan, M. H. A. Ghalia, A. G. E-Amr, and A. H. K. Mohamed, *Anal. Chim. Acta*, 482 (2003) 9
41. R. Yuan, X. L. Wang, L. Xu, Y. Q. Chai, Z. Y. Sun, X. Q. Huang, X. Q. Li, Q. Zhao, and L. Zhou, *Electrochem. Commun.*, 5 (2003) 717
42. M. Mazloum-Ardakani, A. Sadeghi, and M. Salavati-Niassari, *Talanta*, 66 (2005) 837
43. M. Shamsipour, S. Ershad, N. Samadi, A. R. Rezvani, and H. Haddadzadeh, *Talanta*, 65 (2005) 991
44. M. R. Ganjali, H. A. Zamani, and F. Malekzadegan, *Anal. Chim. Acta*, 555 (2006) 336
45. S. Erden, A. Demirel, S. Memon, M. Yılmaz, E. Canel, and E. Kılıç, *Sensor Actuator B*, 113 (2006) 290